

FIG.1

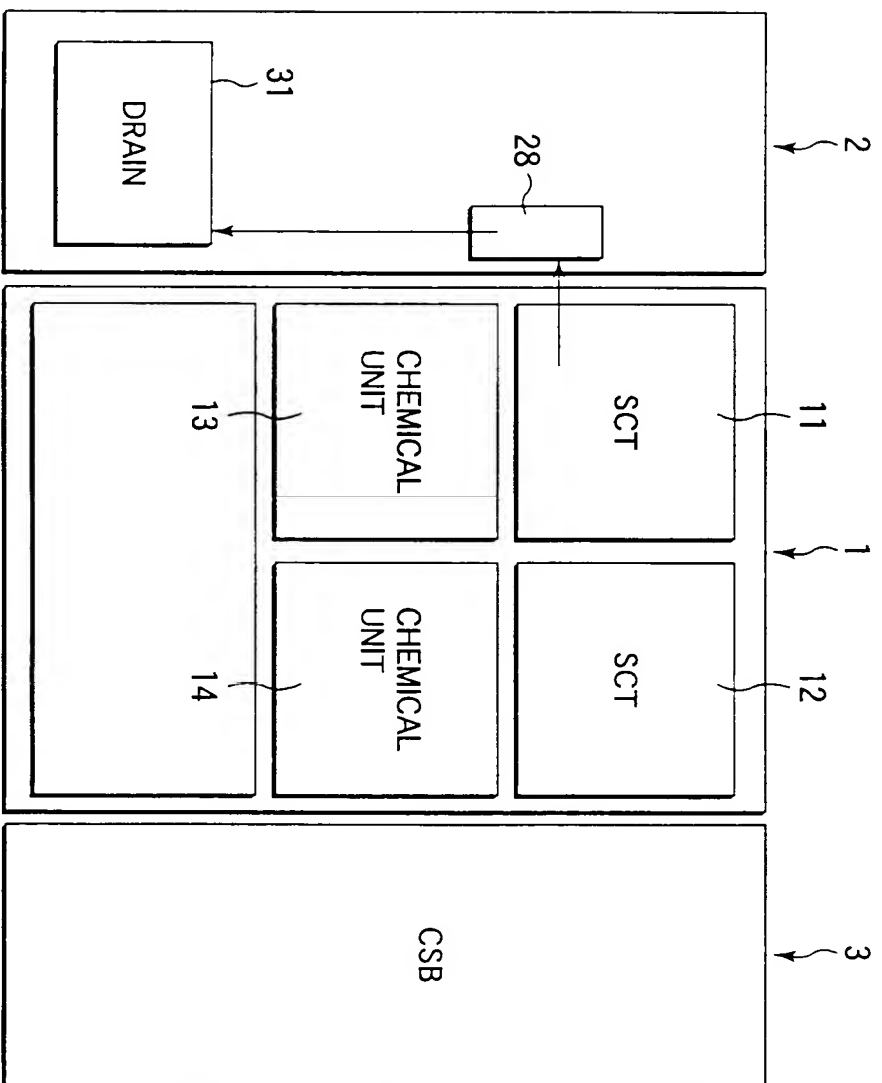


FIG.2

FIG. 3

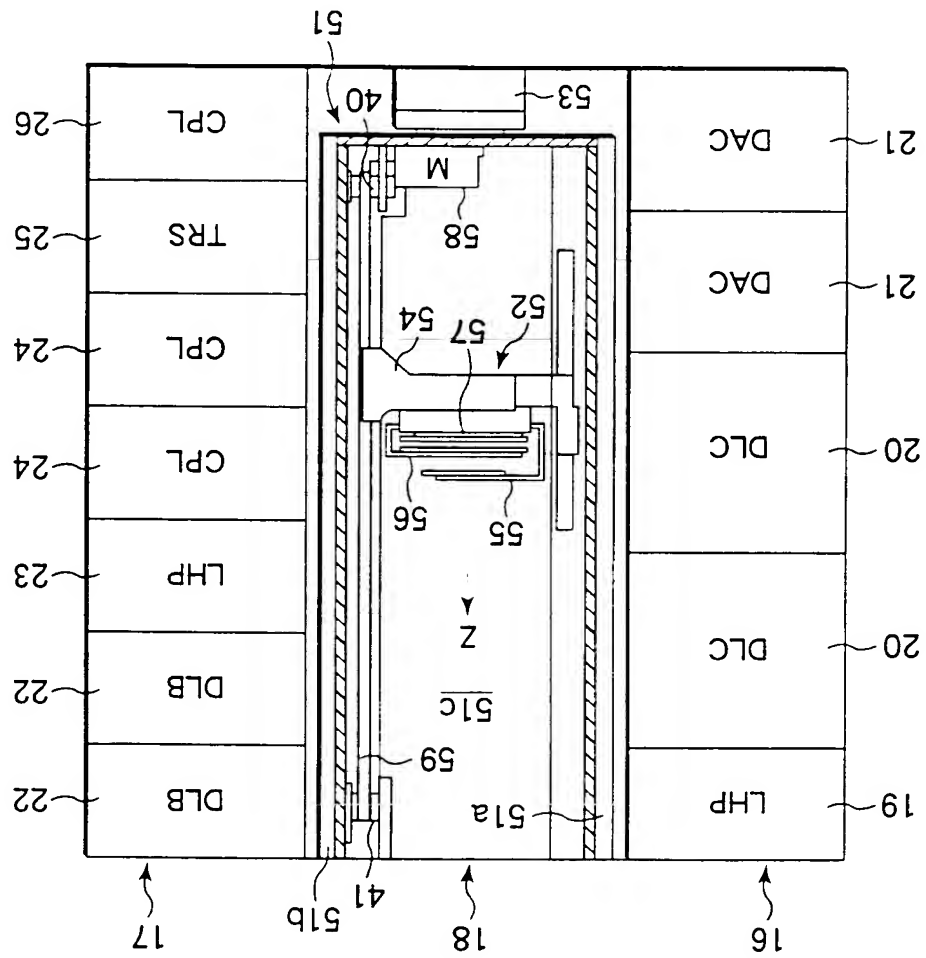
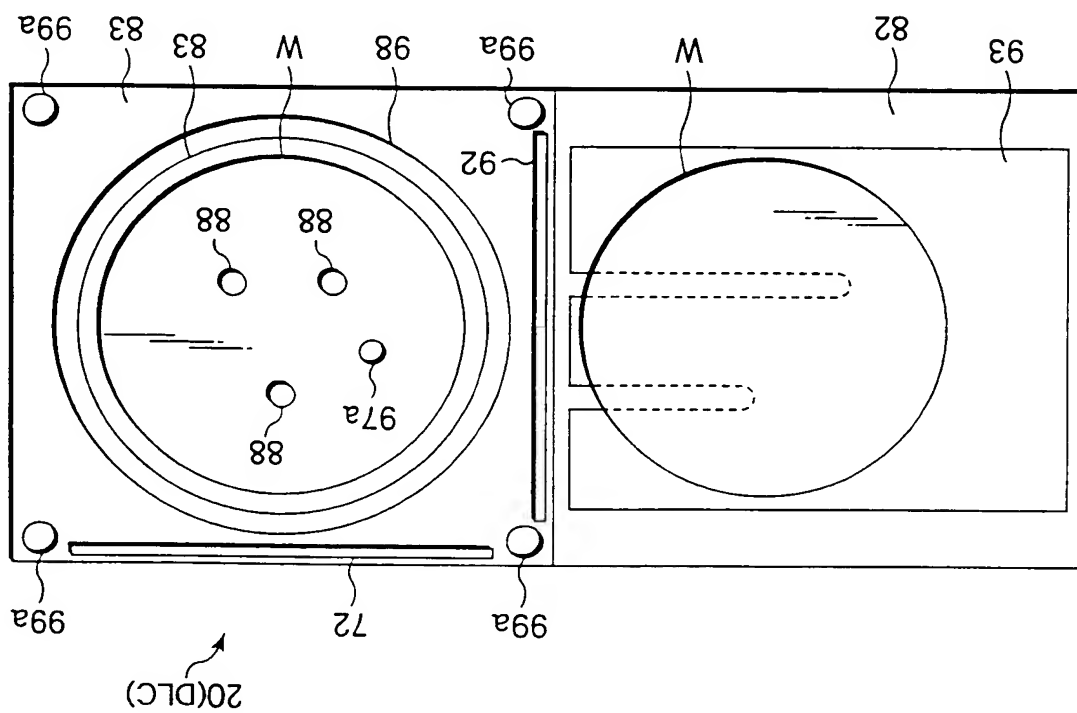


FIG. 4



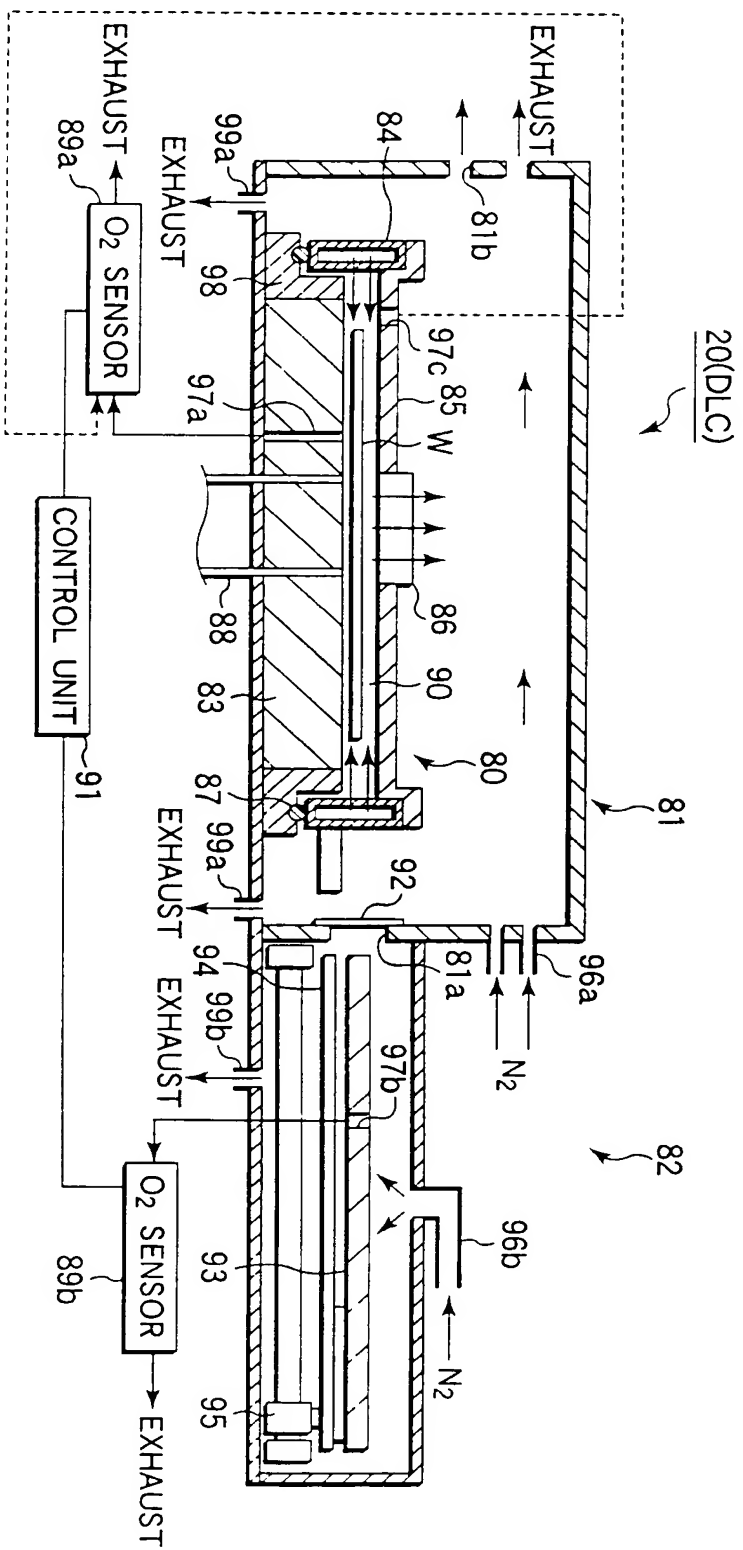


FIG. 6B

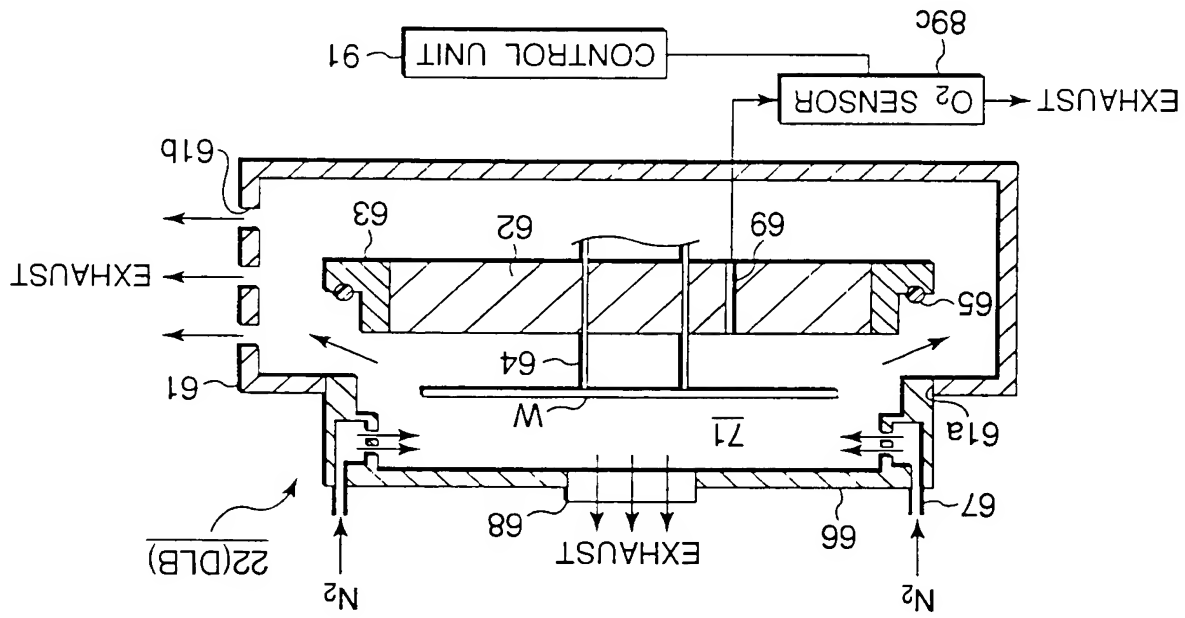


FIG. 6A

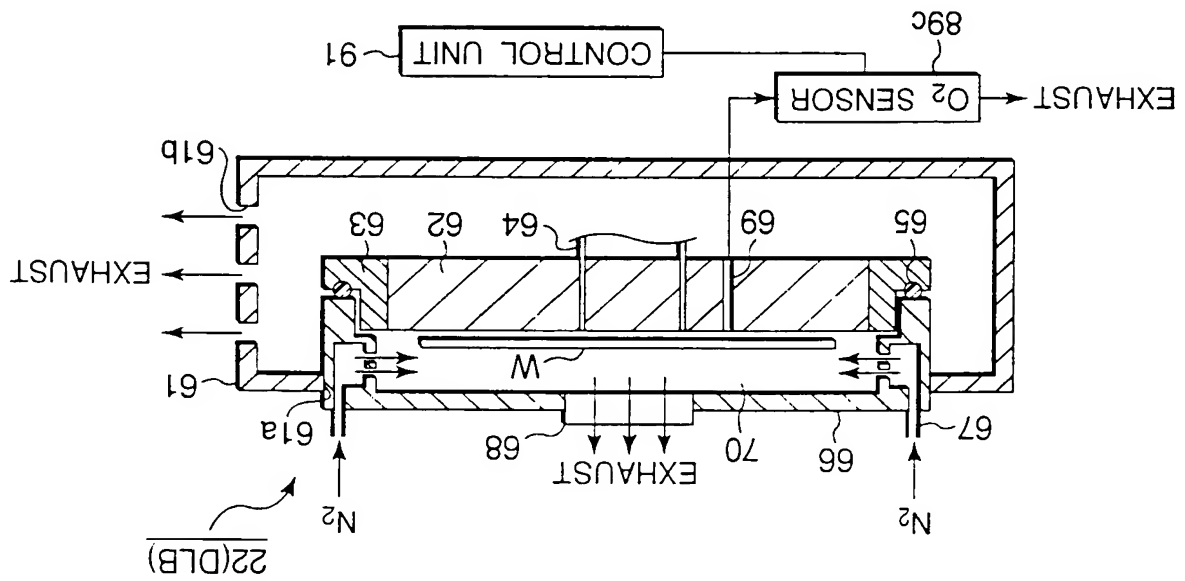


FIG. 7C

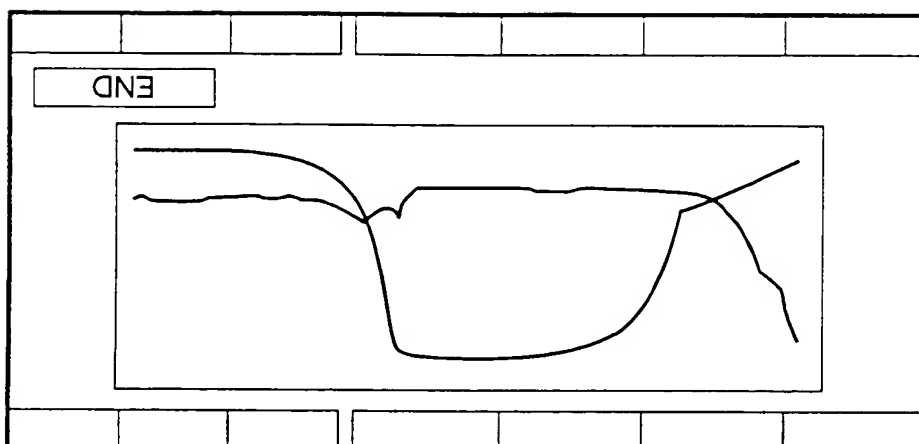


FIG. 7B

START-UP		END	
MEASURING RECIPE →		MEASURING UNIT →	
DLC1		DLC20-1	
DLC2		DLC20-2	

FIG. 7A

OXYGEN CONCENTRATION MEASUREMENT		
.....		
.....		
.....		
.....		

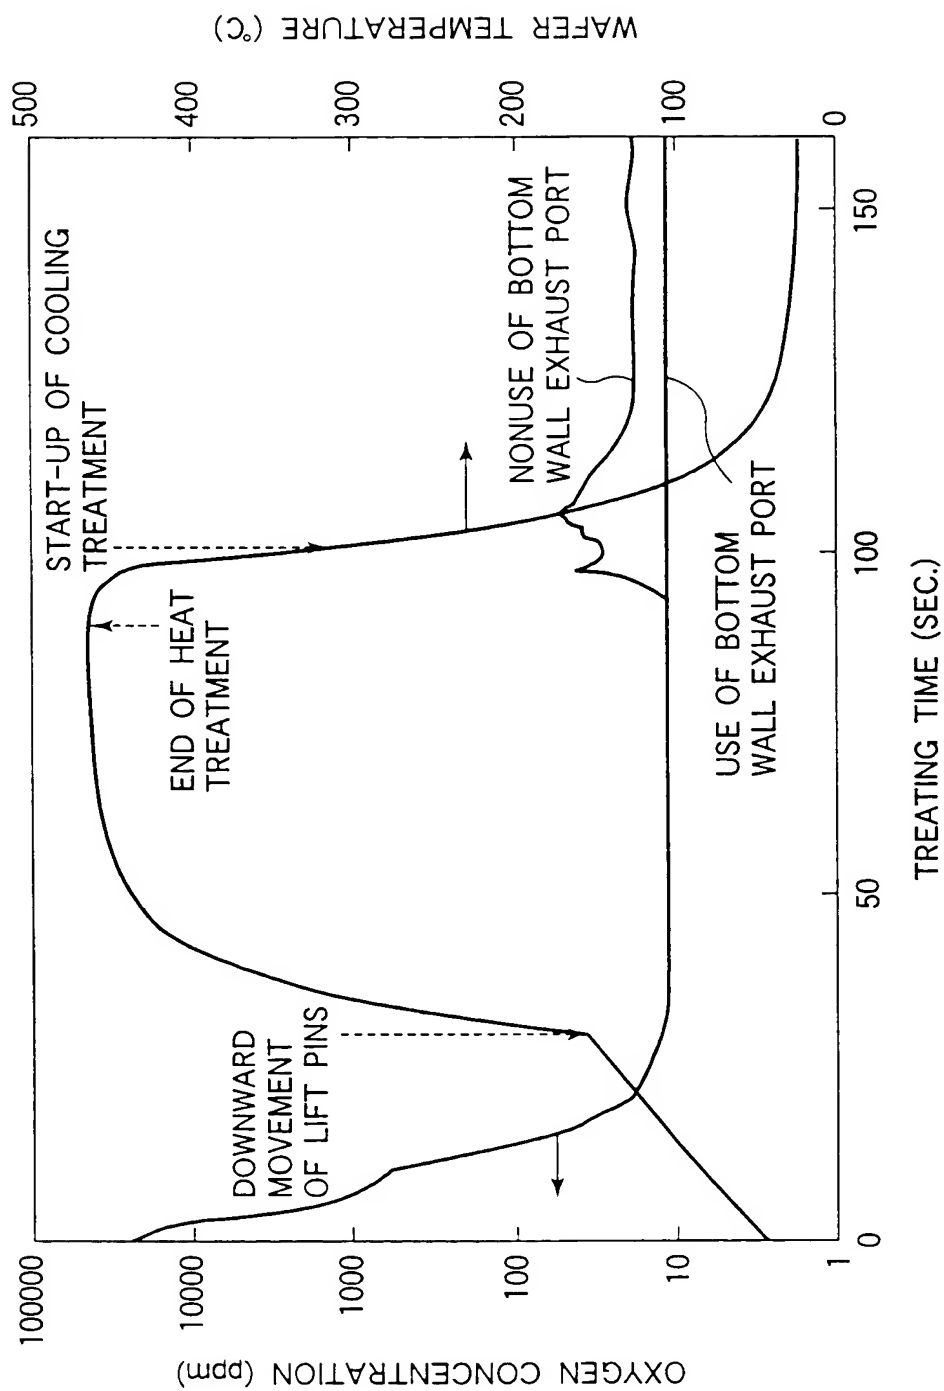


FIG.8



FIG. 9

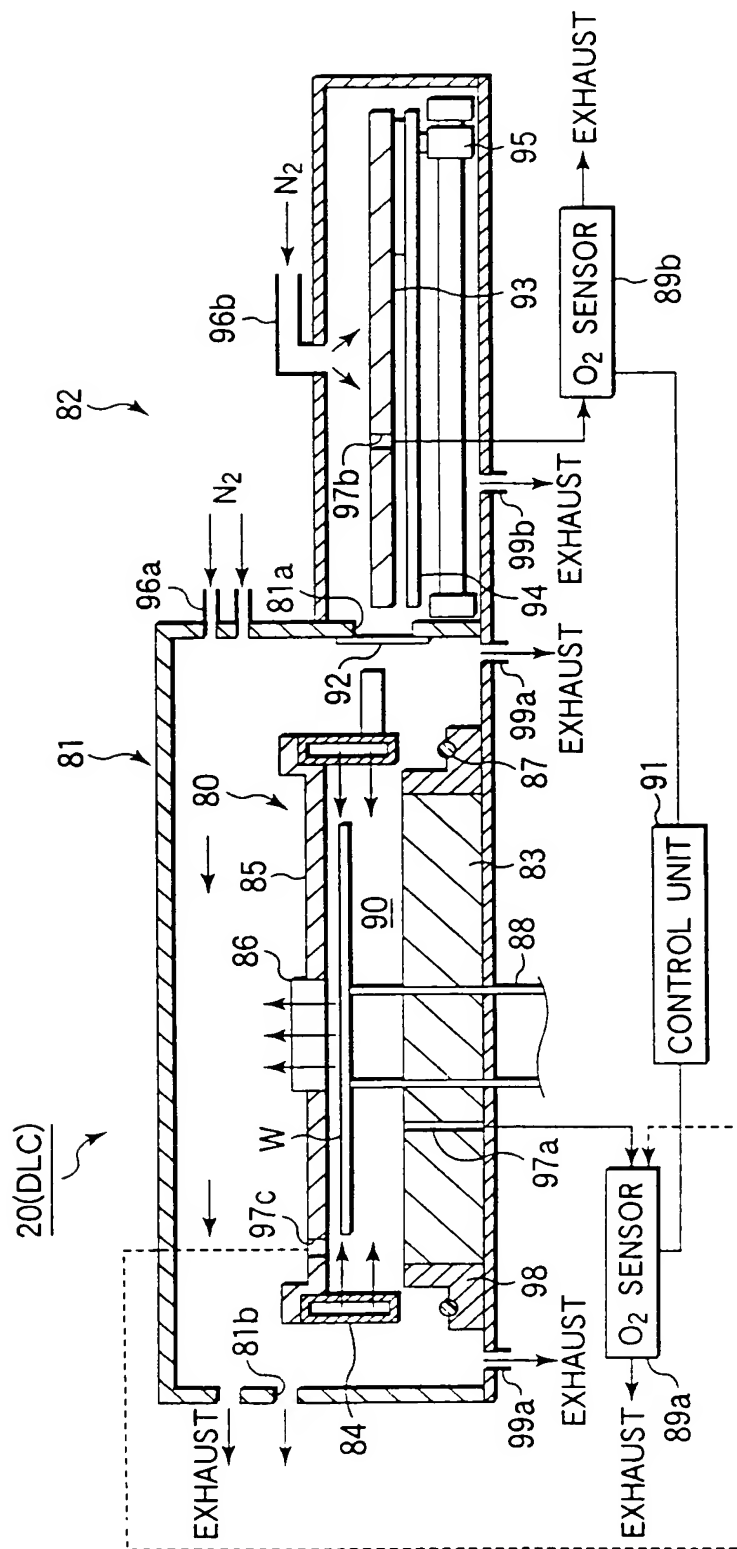


FIG.10

FIG. 11

